

D:\New-nuts\nuts\DATA\SWHL-1-1P9_1.1

11:50:12.022 +0800 NMRSU@EP-10021573

USER: NMRSU

SOLVENT: DMSO

Experiment = zg30

Pulse length = 14.400 usec

Recycle delay = 1.000 sec

NA = 16

Solvent = DMSO

PTS1d = 65536

F1 = 400.140015 MHz

F2 = 1.000000 MHz

SW1 = 8012.82 Hz

AT1 = 8.18 sec

Hz per Pt 1stD = 0.12 Hz

SW2 = 1.00 Hz

Hz per Pt 2ndD = 1.00 Hz

O1 = 2471.5525 Hz



O2 = -1.0000 Hz

LB1 = 0.30 Hz


TP A = 0.00

B = 0.00

C = 0.00

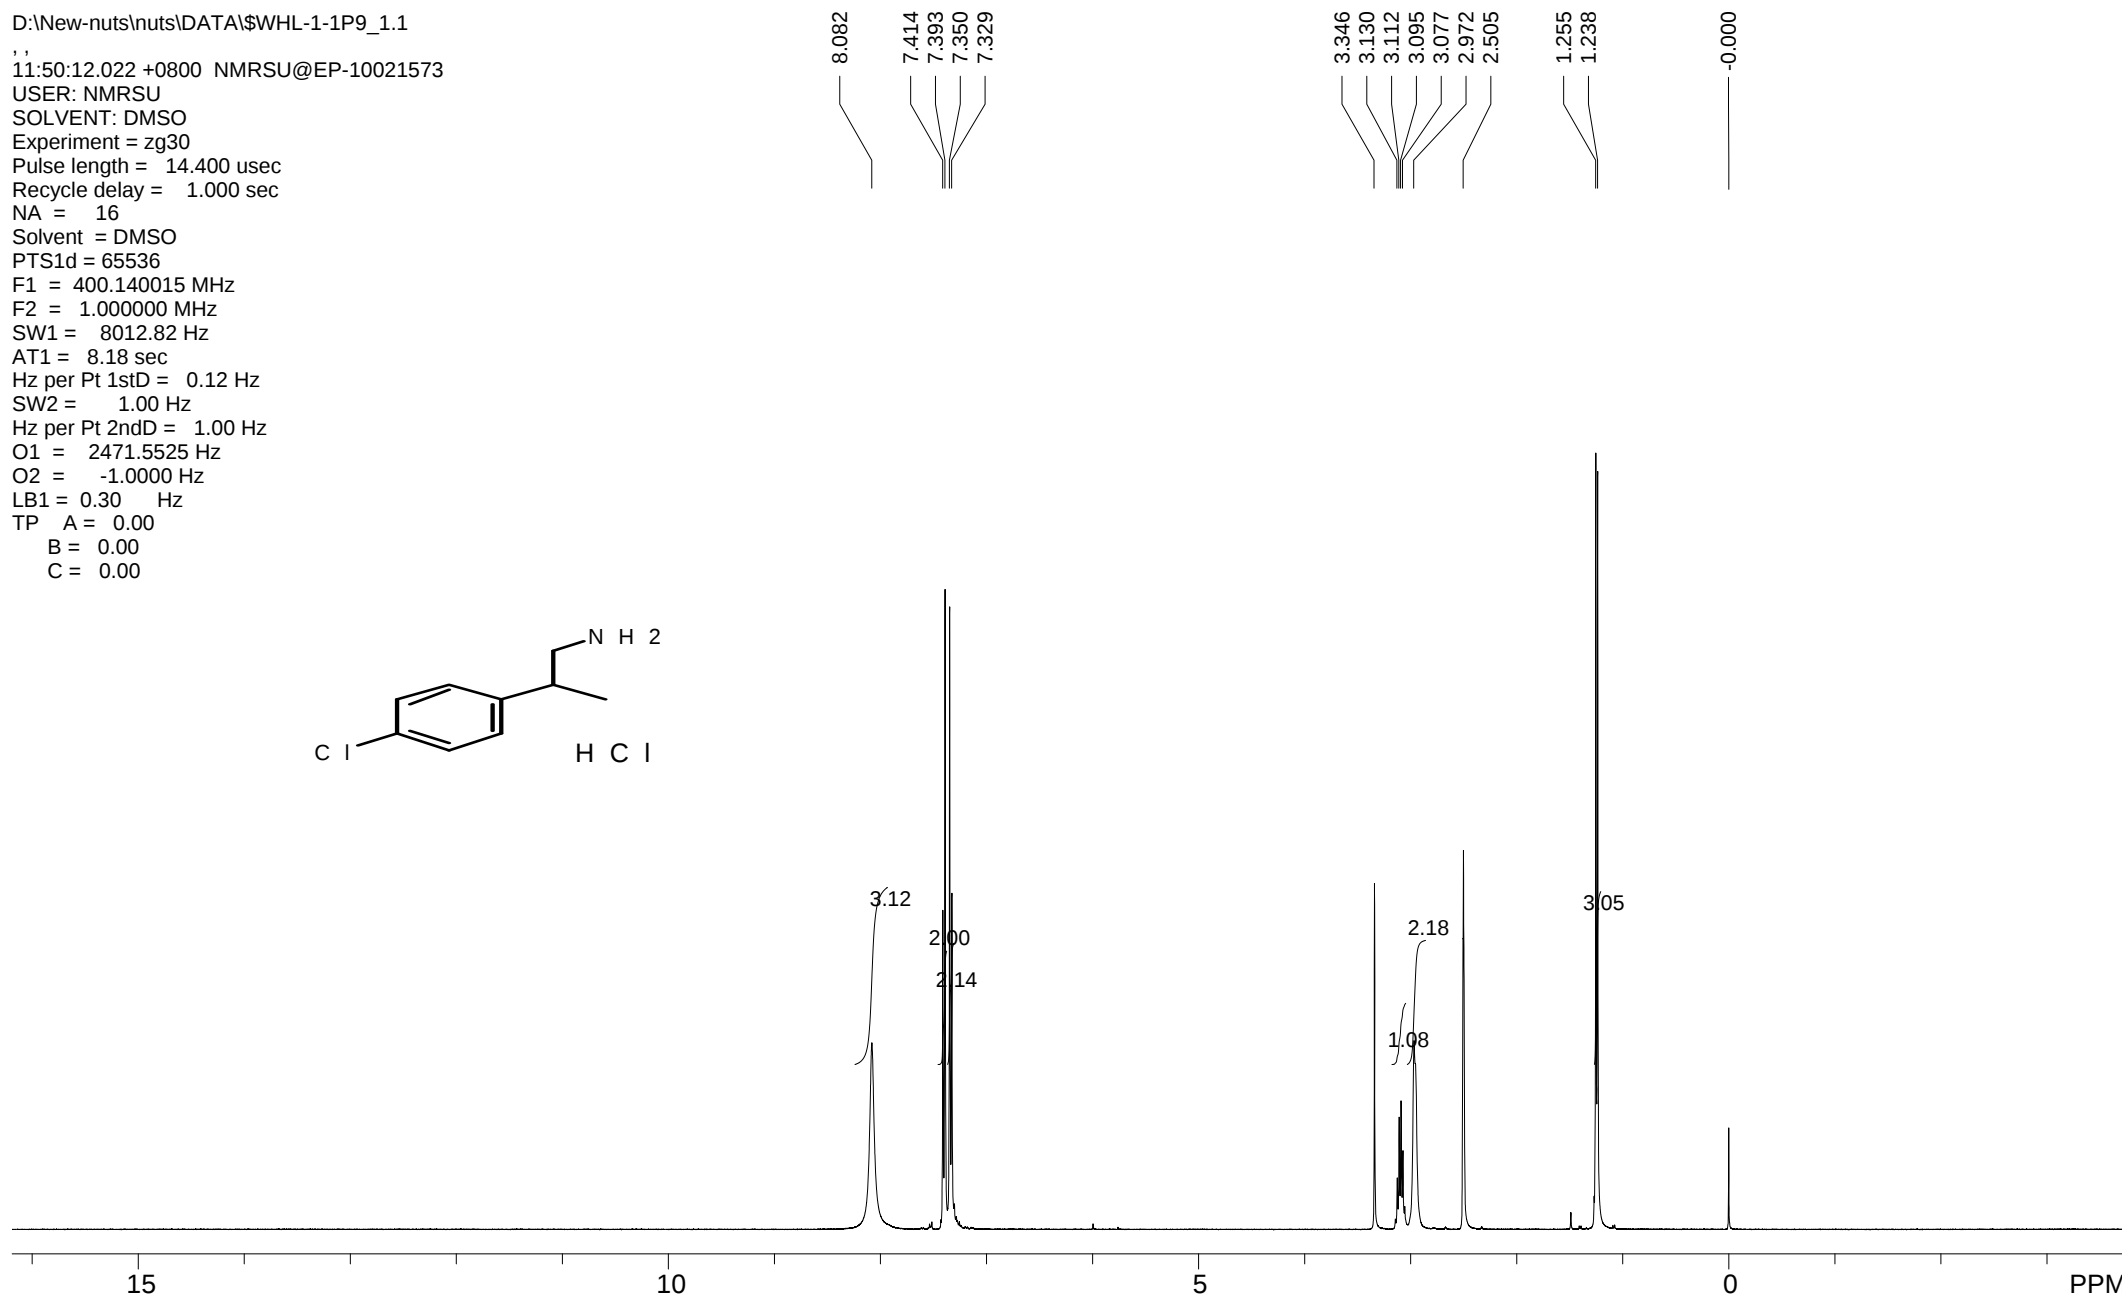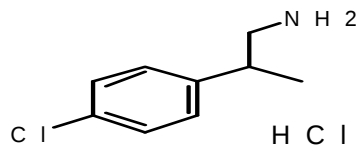

```
=====
Acq. Operator   : SYSTEM                      Seq. Line :    7
Acq. Instrument : HPLC-030                   Location  :   26
Injection Date  : 8/2/2019 11:46:12 AM       Inj       :    1
                                           Inj Volume: 1.000 µl
Different Inj Volume from Sample Entry! Actual Inj Volume : 5.000 µl
Acq. Method     : D:\HPLC-030\Data\2019\20190801-1 2019-08-02 09-32-12\M-A80B20.M
Last changed    : 8/2/2019 10:18:58 AM by SYSTEM
Analysis Method : D:\HPLC-030\METHODS\SUNFIRE C18 5UM 4.6X150MM\M-AB.M
Last changed    : 8/2/2019 12:49:48 PM by SYSTEM
Method Info     : SunFire C18 5um 4.6x150mm 25C 1.000ml/min 16min
                  Mobile Phase A: 0.03%TFA in H2O, Mobile Phase B: 0.03%TFA in ACN.
=====
```

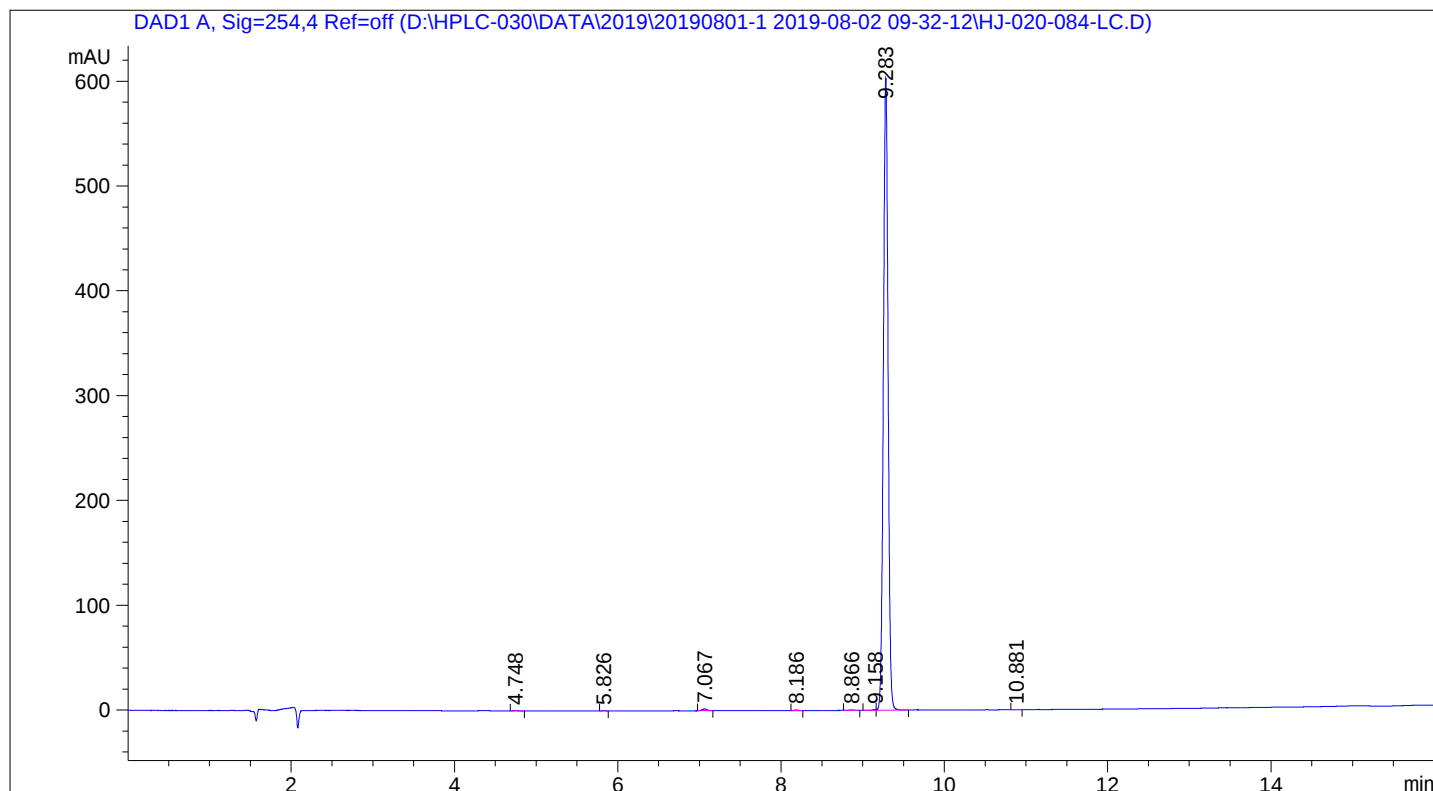

```
=====
Area Percent Report
=====
```

```
Sorted By      : Signal
Multiplier     : 1.0000
Dilution       : 1.0000
Do not use Multiplier & Dilution Factor with ISTDs
```


Signal 1: DAD1 A, Sig=254,4 Ref=off

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	4.748	BB	0.0479	6.81710e-1	1.77322e-1	0.0282
2	5.826	BB	0.0408	4.45223e-1	1.39204e-1	0.0184
3	7.067	BB	0.0610	6.86698	1.68519	0.2839
4	8.186	BB	0.0492	1.68862	5.09504e-1	0.0698
5	8.866	BB	0.0630	2.40282	5.33945e-1	0.0993
6	9.158	BV	0.0467	2.20025	6.99820e-1	0.0910
7	9.283	VB	0.0620	2403.69678	603.11536	99.3852
8	10.881	BB	0.0542	5.83305e-1	1.36870e-1	0.0241

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
----- ----- ----- ----- ----- ----- -----						
Totals :				2418.56569	606.99721	

=====
*** End of Report ***

```
=====
Acq. Operator   : SYSTEM                      Seq. Line :    7
Acq. Instrument : HPLC-030                   Location  :   26
Injection Date  : 8/2/2019 11:46:12 AM        Inj       :    1
                                           Inj Volume: 1.000 µl
Different Inj Volume from Sample Entry! Actual Inj Volume : 5.000 µl
Acq. Method     : D:\HPLC-030\Data\2019\20190801-1 2019-08-02 09-32-12\M-A80B20.M
Last changed    : 8/2/2019 10:18:58 AM by SYSTEM
Analysis Method : D:\HPLC-030\METHODS\SUNFIRE C18 5UM 4.6X150MM\M-AB.M
Last changed    : 8/2/2019 12:50:54 PM by SYSTEM
Method Info     : SunFire C18 5um 4.6x150mm 25C 1.000ml/min 16min
                  Mobile Phase A: 0.03%TFA in H2O, Mobile Phase B: 0.03%TFA in ACN.
=====
```

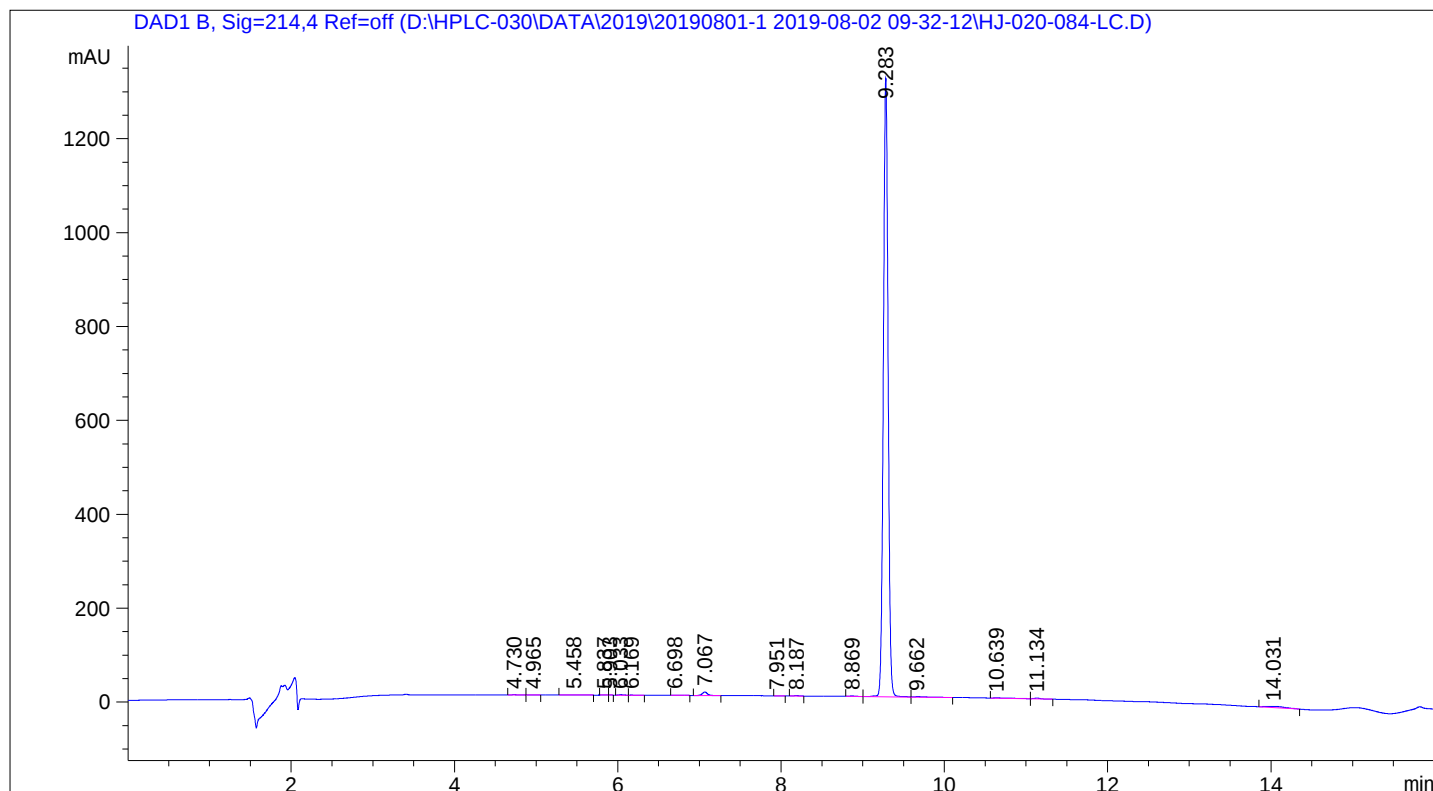

Area Percent Report

```
Sorted By      : Signal
Multiplier     : 1.0000
Dilution      : 1.0000
Do not use Multiplier & Dilution Factor with ISTDs
```

Signal 1: DAD1 B, Sig=214,4 Ref=off

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	4.730	BB	0.0580	2.90689	7.21916e-1	0.0536
2	4.965	BB	0.0544	9.49832e-1	2.15490e-1	0.0175
3	5.458	BB	0.1356	6.01075	5.24747e-1	0.1109
4	5.837	BV	0.0463	8.48439e-1	2.31370e-1	0.0157
5	5.903	VB	0.0315	2.61447e-1	1.07064e-1	4.825e-3
6	6.033	BV	0.0446	3.37677	1.09051	0.0623
7	6.169	VB	0.0604	1.24288	2.57013e-1	0.0229
8	6.698	BB	0.0605	1.44405	2.92987e-1	0.0266

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
9	7.067	BB	0.0634	30.90210	7.45462	0.5703
10	7.951	BB	0.0498	5.37109e-1	1.35269e-1	9.912e-3
11	8.187	BB	0.0523	3.30541	9.69805e-1	0.0610
12	8.869	BV	0.0748	4.45059	8.08028e-1	0.0821
13	9.283	VV	0.0623	5289.77979	1317.97168	97.6178
14	9.662	VB	0.1501	12.29677	9.78569e-1	0.2269
15	10.639	BV	0.1776	11.41309	8.06274e-1	0.2106
16	11.134	VBA	0.0876	9.85475	1.68909	0.1819
17	14.031	BBA	0.1985	39.28933	2.38083	0.7250

Totals : 5418.87000 1336.63525

=====
*** End of Report ***