
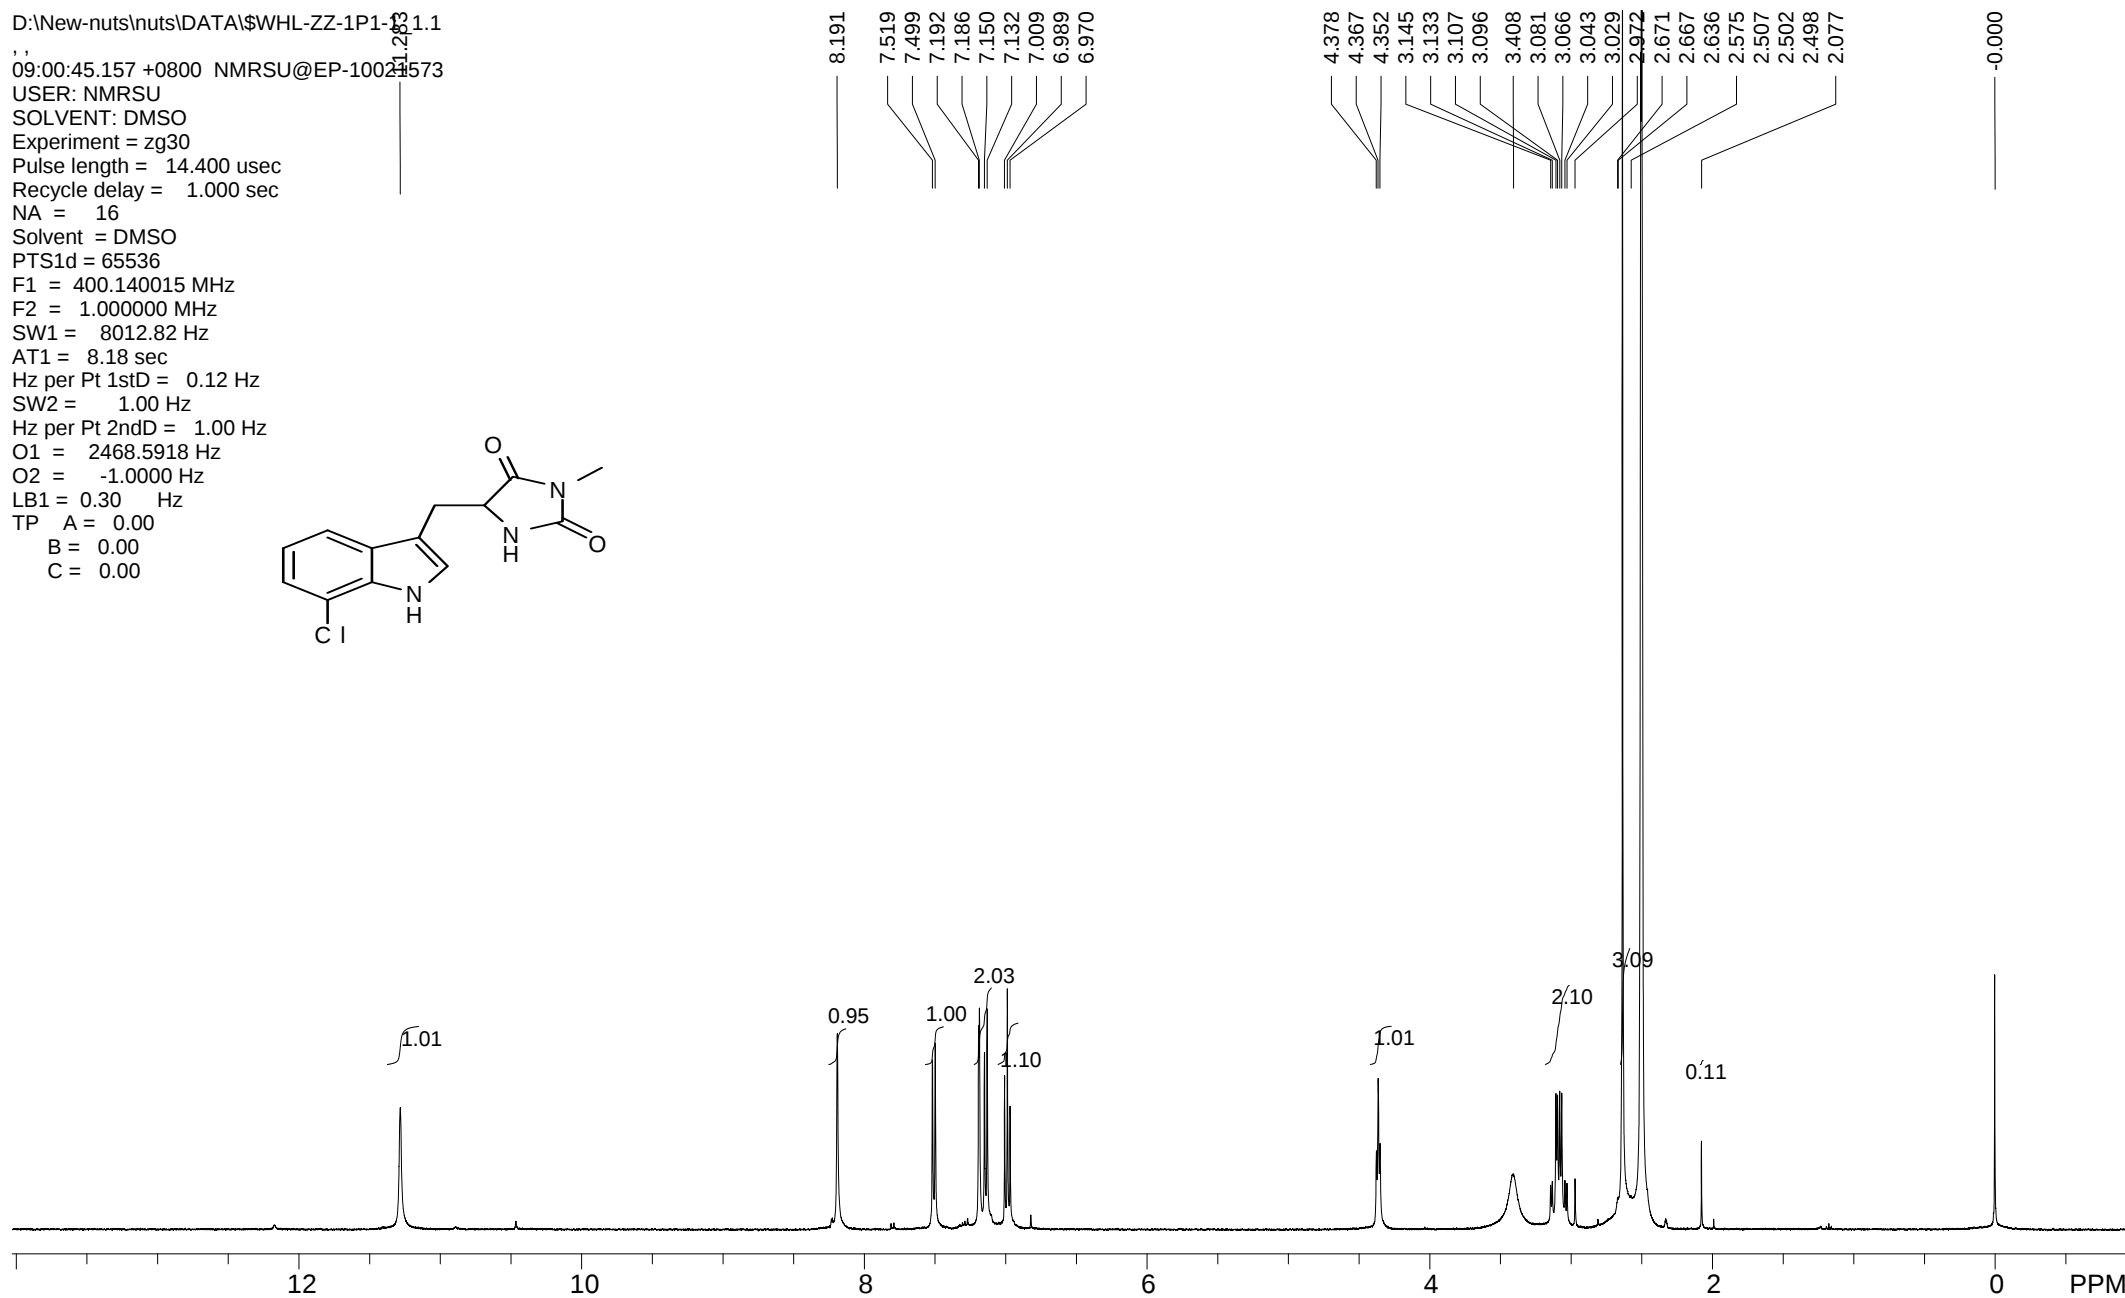


D:\New-nuts\nuts\DATA\SWHL-ZZ-1P1-11.1
 09:00:45.157 +0800 NMRSU@EP-10021573
 USER: NMRSU
 SOLVENT: DMSO
 Experiment = zg30
 Pulse length = 14.400 usec
 Recycle delay = 1.000 sec
 NA = 16
 Solvent = DMSO
 PTS1d = 65536
 F1 = 400.140015 MHz
 F2 = 1.000000 MHz
 SW1 = 8012.82 Hz
 AT1 = 8.18 sec
 Hz per Pt 1stD = 0.12 Hz
 SW2 = 1.00 Hz
 Hz per Pt 2ndD = 1.00 Hz
 O1 = 2468.5918 Hz
 O2 = -1.0000 Hz
 LB1 = 0.30 Hz
 TP A = 0.00
 B = 0.00
 C = 0.00

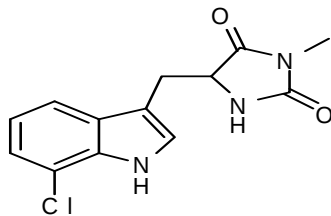

HPLC Report

<Sample Information>

Sample Name	: MC19-03-023-P1	Method Filename	: HILIC-H0-A5B95.lcm
Data Filename	: MC19-03-023-P1-LC.lcd	Vial #	: 1-59
Batch Filename	: 20190410.lcb	Injection Volume	: 1 uL
Date Acquired	: 4/10/2019 1:48:04 PM	Acquired by	: System Administrator
Date Processed	: 4/10/2019 2:07:46 PM	Processed by	: System Administrator


Atlatis HILIC Silica 5um 4.6x150mm 25C 1.000ml/min 16min

<<Mobile Phase Name>>

Pump A Mobile Phase A	: 0.03%TFA in H2O
Pump B Mobile Phase A	: 0.03%TFA in ACN

<Chromatogram>

mV

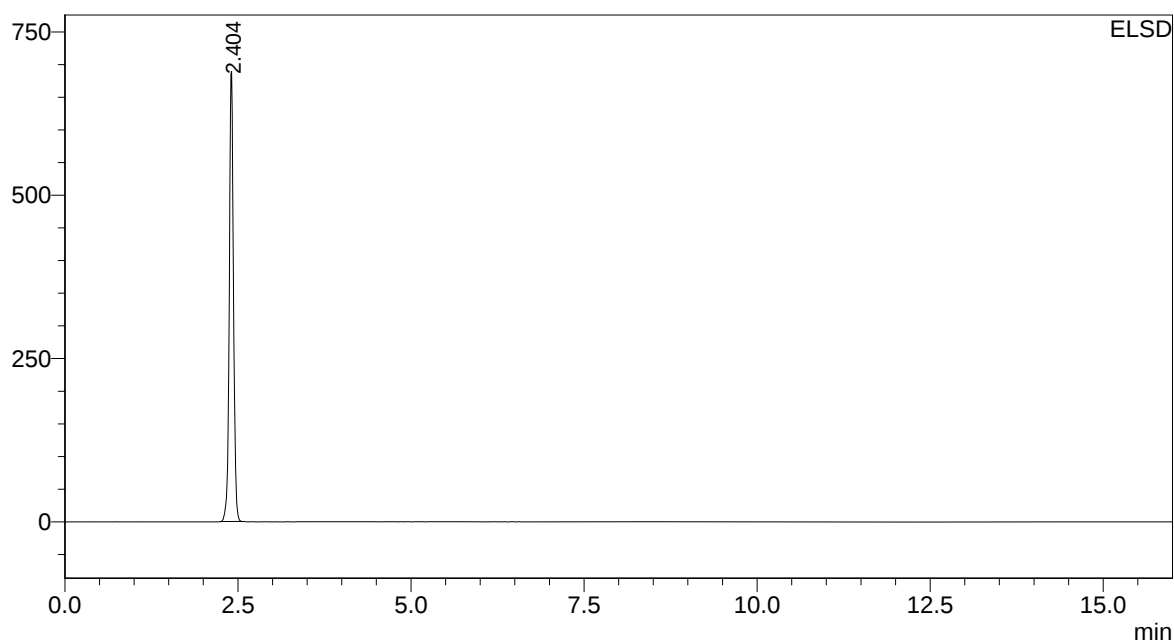

<Peak Table>

ELSD						
Peak#	Ret. Time	USP Width	Height	Area	S/N	Area%
1	2.404	0.122	654937	2901382	4329.05	100.000
Total				2901382		100.000

HPLC Report

<Sample Information>

Sample Name	: MC19-03-023-P1	Method Filename	: HILIC-H0-A5B95.lcm
Data Filename	: MC19-03-023-P1-LC.lcd	Vial #	: 1-59
Batch Filename	: 20190410.lcb	Injection Volume	: 1 uL
Date Acquired	: 4/10/2019 1:48:04 PM	Acquired by	: System Administrator
Date Processed	: 4/10/2019 2:07:03 PM	Processed by	: System Administrator


Atlatis HILIC Silica 5um 4.6x150mm 25C 1.000ml/min 16min

<<Mobile Phase Name>>

Pump A Mobile Phase A	: 0.03%TFA in H2O
Pump B Mobile Phase A	: 0.03%TFA in ACN

<Chromatogram>

mAU

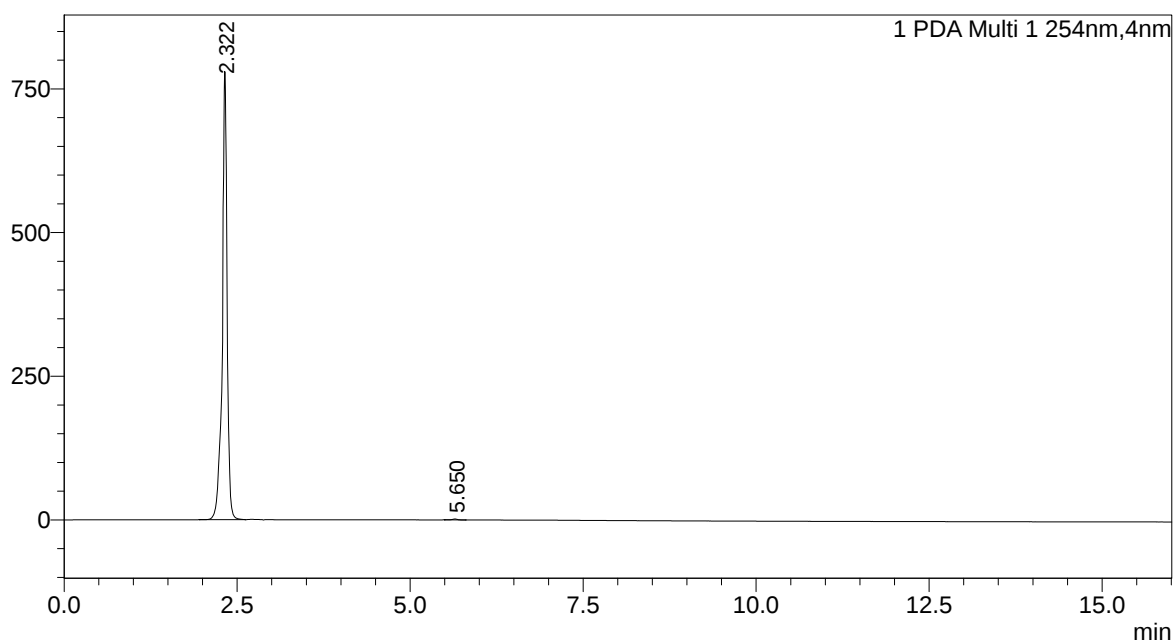

<Peak Table>

PDA Ch1 254nm

Peak#	Ret. Time	USP Width	Height	Area	S/N	Area%
1	2.322	0.120	780152	3760950	10368.57	99.785
2	5.650	0.134	1598	8090	21.24	0.215
Total				3769040		100.000

Shimadzu MS-002 Report

Sample Information

LCMS
Sample Name : WHL-ZZ-9-RP15 Date Acquired : 2019-04-10 07:26:35
Injection Volume : 10 Tray# : 1
Vial# : 42 Method File : A60B40+-.lcm

Column :

Mass Spectrum

Rt=1.063min Positive

