

D:\New-nuts\nuts\DATA\SWHL-100-P-6-9_1.1

07:18:46.403 +0800 NMRSU@EP-10021573

USER: NMRSU

SOLVENT: DMSO

Experiment = zg30

Pulse length = 14.000 usec

Recycle delay = 1.000 sec

NA = 8

Solvent = DMSO

PTS1d = 65536

F1 = 400.139954 MHz

F2 = 1.000000 MHz

SW1 = 8012.82 Hz

AT1 = 8.18 sec

Hz per Pt 1stD = 0.12 Hz

SW2 = 1.00 Hz

Hz per Pt 2ndD = 1.00 Hz

O1 = 2504.0190 Hz



O2 = -1.0000 Hz

LB1 = 0.30 Hz


TP A = 0.00

B = 0.00

C = 0.00

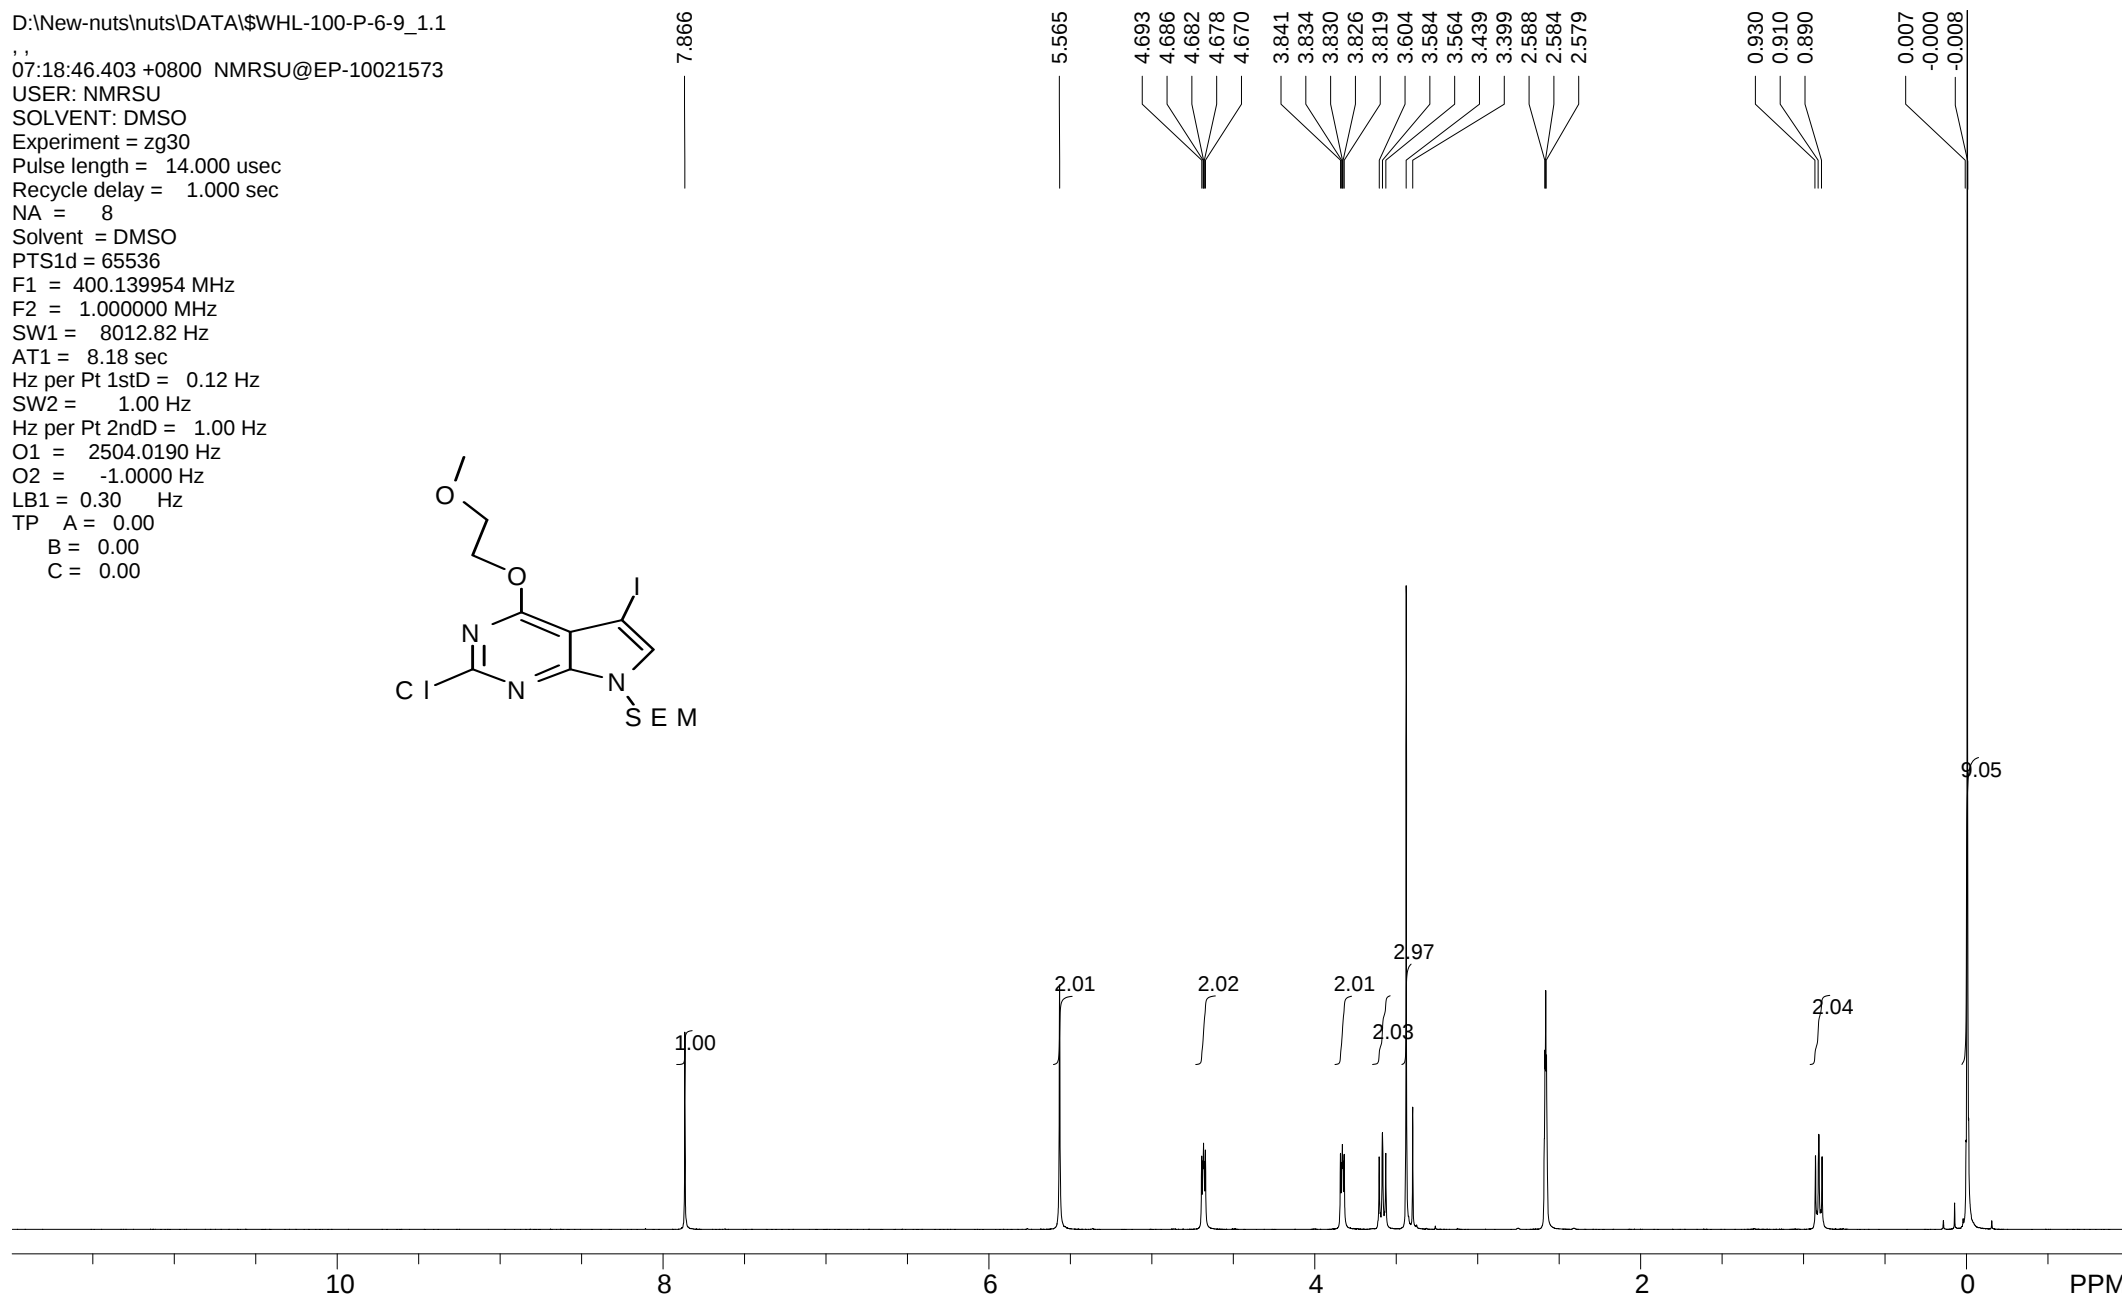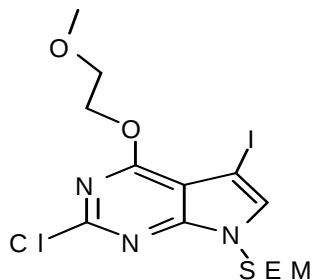

```
=====
Acq. Operator   : SYSTEM                      Seq. Line :    2
Acq. Instrument : HPLC-030                   Location  :   39
Injection Date  : 3/26/2019 10:25:13 AM      Inj       :    1
                                           Inj Volume: 10.000 µl
Different Inj Volume from Sample Entry! Actual Inj Volume : 2.000 µl
Acq. Method     : D:\HPLC-030\Data\2019\20190326 2019-03-26 09-52-36\M-A20B80.M
Last changed    : 3/26/2019 9:55:26 AM by SYSTEM
Analysis Method : D:\HPLC-030\METHODS\SUNFIRE C18 5UM 4.6X150MM\M-AB.M
Last changed    : 3/26/2019 10:58:20 AM by SYSTEM
Method Info     : SunFire C18 5um 4.6x150mm 25C 1.000ml/min 16min
                  Mobile Phase A: 0.03%TFA in H2O, Mobile Phase B: 0.03%TFA in ACN.
=====
```

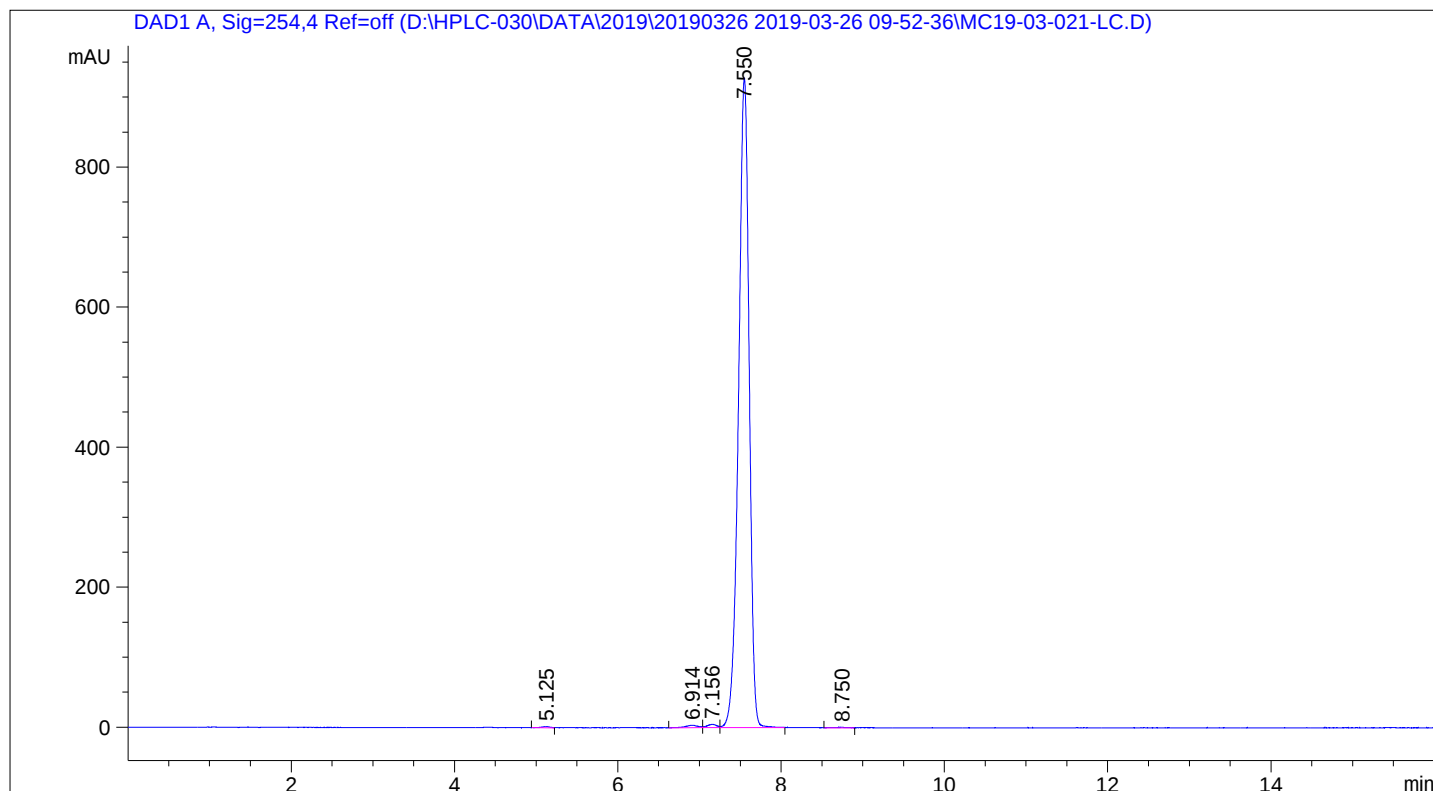

```
=====
                          Area Percent Report
=====
```

```
Sorted By      :      Signal
Multiplier     :      1.0000
Dilution       :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs
```


Signal 1: DAD1 A, Sig=254,4 Ref=off

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	5.125	BV	0.0832	11.97320	1.76478	0.1415
2	6.914	BV	0.1307	37.85229	3.54076	0.4472
3	7.156	VV	0.1091	39.23810	4.81374	0.4636
4	7.550	VB	0.1382	8368.82617	927.93005	98.8695
5	8.750	BB	0.1363	6.63042	6.12682e-1	0.0783

Totals : 8464.52019 938.66202

=====
*** End of Report ***

```
=====
Acq. Operator   : SYSTEM                      Seq. Line :    2
Acq. Instrument : HPLC-030                   Location  :   39
Injection Date  : 3/26/2019 10:25:13 AM      Inj       :    1
                                           Inj Volume: 10.000 µl
Different Inj Volume from Sample Entry! Actual Inj Volume : 2.000 µl
Acq. Method     : D:\HPLC-030\Data\2019\20190326 2019-03-26 09-52-36\M-A20B80.M
Last changed    : 3/26/2019 9:55:26 AM by SYSTEM
Analysis Method : D:\HPLC-030\METHODS\SUNFIRE C18 5UM 4.6X150MM\M-AB.M
Last changed    : 3/26/2019 10:59:13 AM by SYSTEM
Method Info     : SunFire C18 5um 4.6x150mm 25C 1.000ml/min 16min
                  Mobile Phase A: 0.03%TFA in H2O, Mobile Phase B: 0.03%TFA in ACN.
=====
```

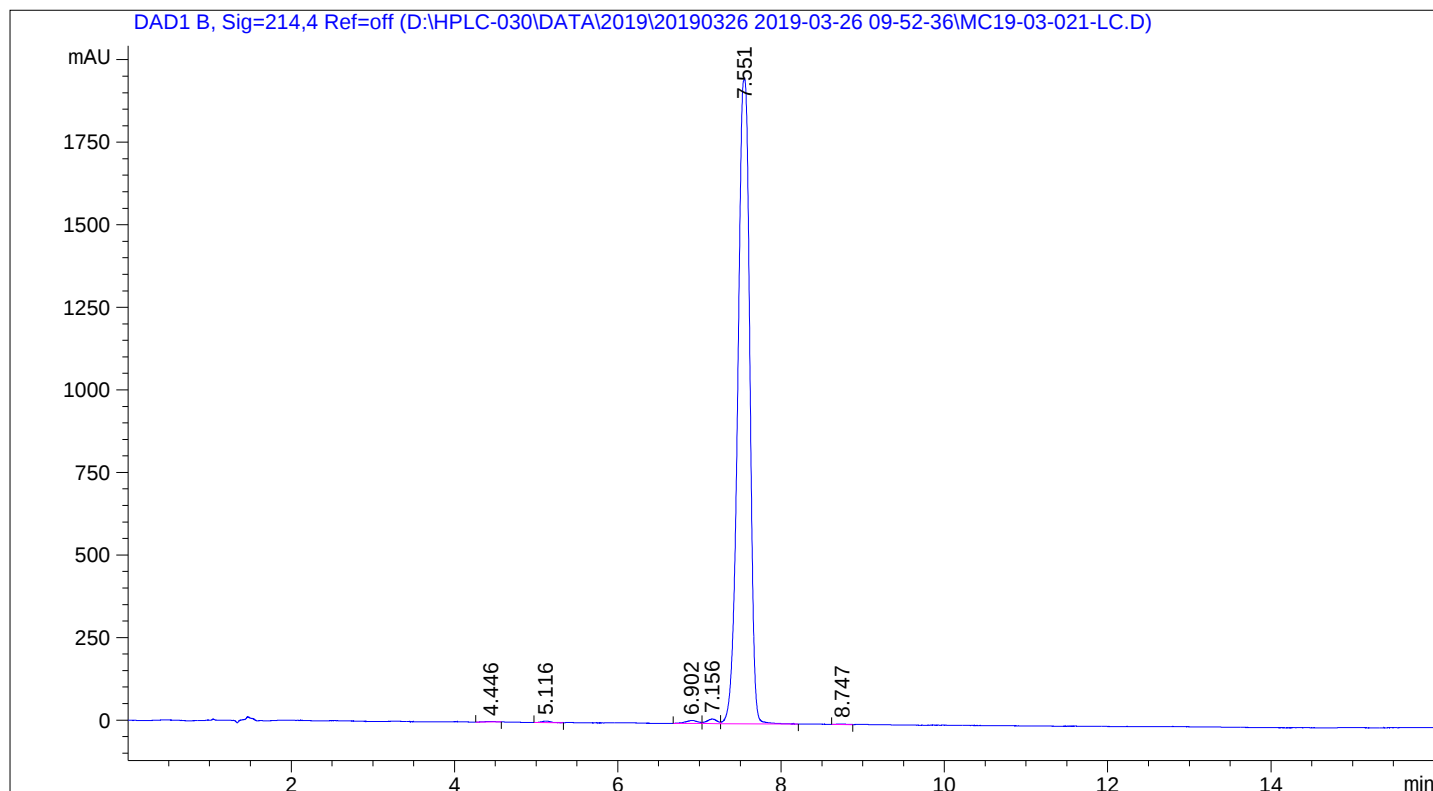

=====
Area Percent Report
=====

```
Sorted By      : Signal
Multiplier     : 1.0000
Dilution       : 1.0000
Do not use Multiplier & Dilution Factor with ISTDs
```

Signal 1: DAD1 B, Sig=214,4 Ref=off

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	4.446	BB	0.1118	17.70763	1.91663	0.0884
2	5.116	BB	0.0884	32.44295	4.59123	0.1621
3	6.902	BV	0.1306	94.47108	9.13863	0.4719
4	7.156	VV	0.1237	116.72083	13.79937	0.5830
5	7.551	VB	0.1379	1.97479e4	1954.93311	98.6410
6	8.747	BB	0.0910	10.72240	1.42107	0.0536

Totals : 2.00200e4 1985.80003

=====
*** End of Report ***

Shimadzu MS-017 Report

Sample Information

LCMS

Sample Name : WHL-100-P6

Date Acquired : 2019-03-26 07:55:09

Injection Volume : 5

Tray# : 1

Vial# : 57

Method File : A40B60.lcm

Column : SunFire C18 50*4.6mm 5um 2.000ml/min 2.6min

Pump A : 0.1%FA-H2O

Pump B : 0.1%FA-ACN

Mass Spectrum

RT=2.040 Positive

